

Applicant(s): Frederick Geheb
CARDIO-PULMONARY RESUSCITATION DEVICE WITH
FEEDBACK FROM MEASUREMENT OF PULSE AND/OR
BLOOD OXYGENATION

FIGURE 1

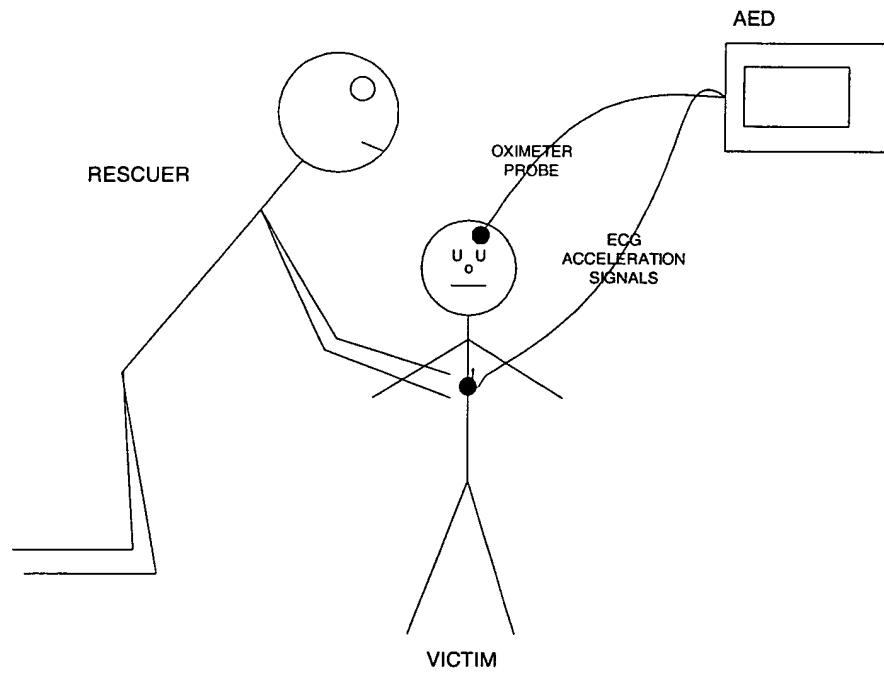


FIGURE 2

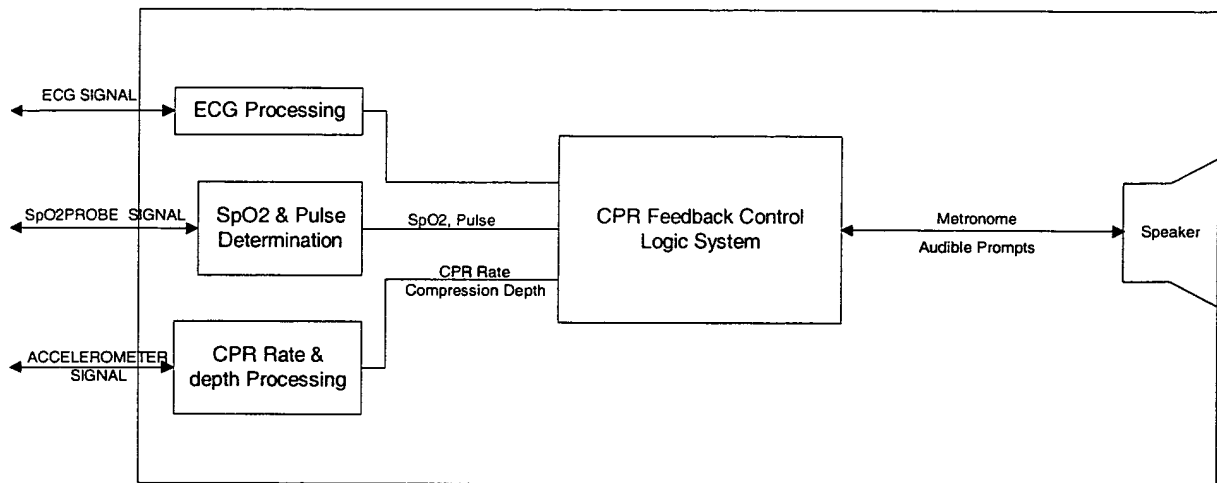


FIGURE 3

